



## Operation Equipment Key




## Stage 1: Loading bung device

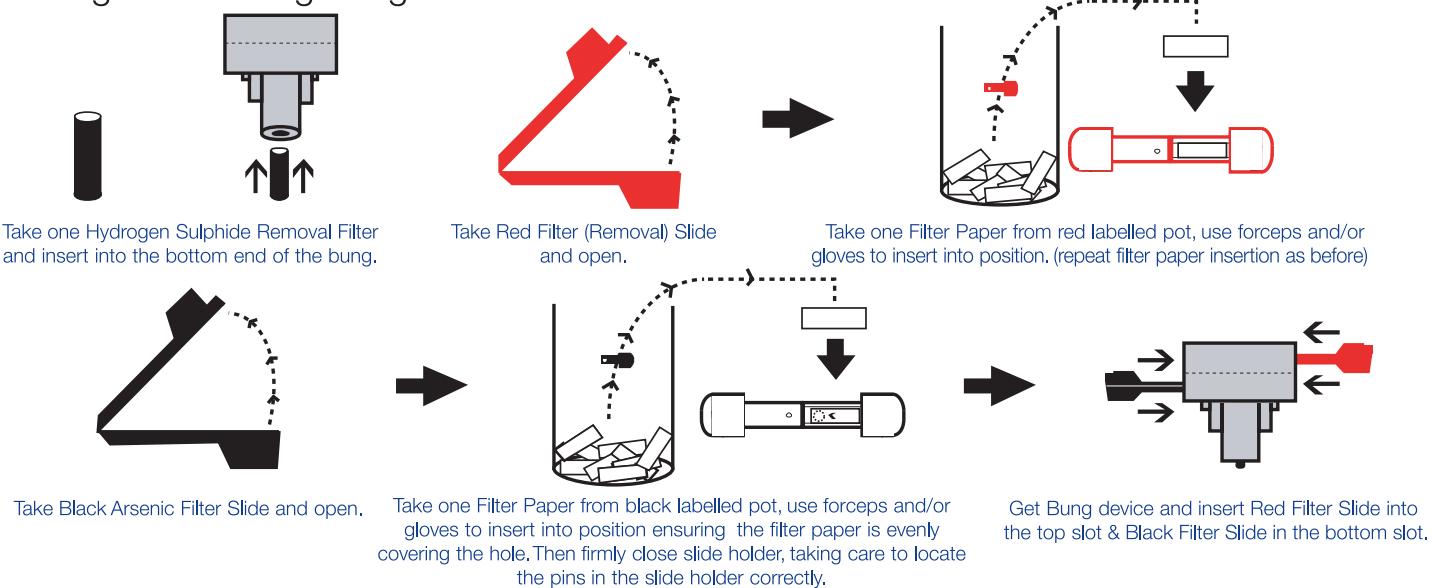


## Stage 2: Sample Preparation

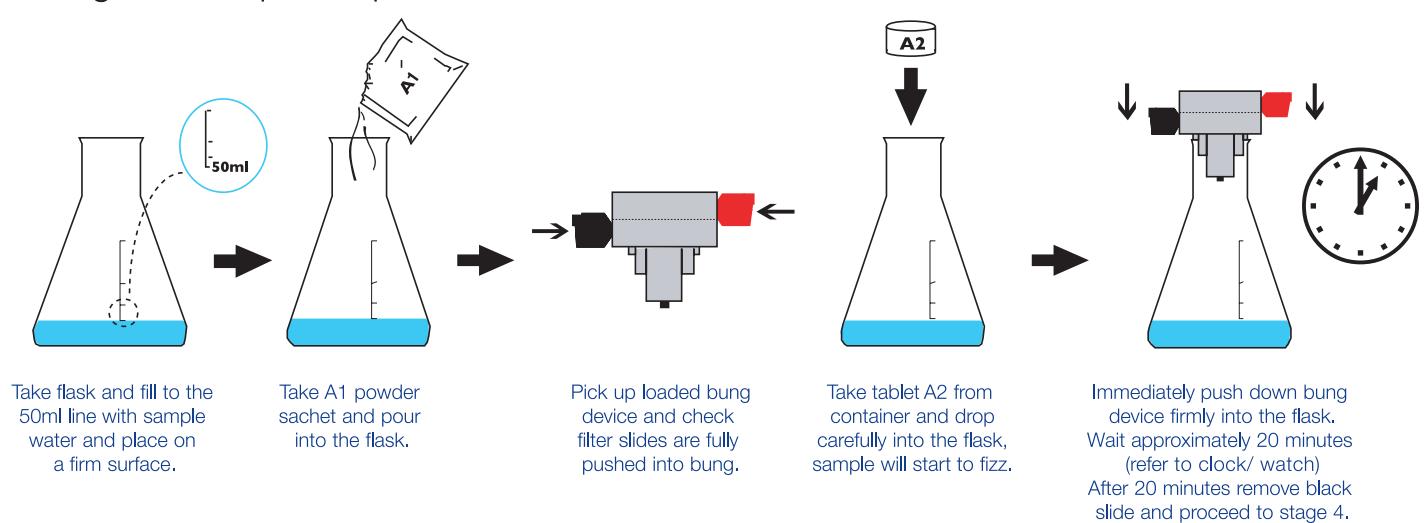




## Stage 3: Arsenic Measurement (colour comparison - using the colour chart)

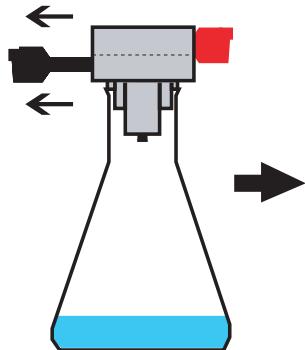

Remove Black Filter Slide  
from Bung device.




Record corresponding Colour, Match from colour chart  
to obtain result in µg/l (ppb).



If test result reads above 500µg/l (ppb) use dilution  
tube with de-ionised water and convert accordingly.  
Then go back to stage 1 and do test again.

For Verification of readings  
less than 100µg/l (ppb)...

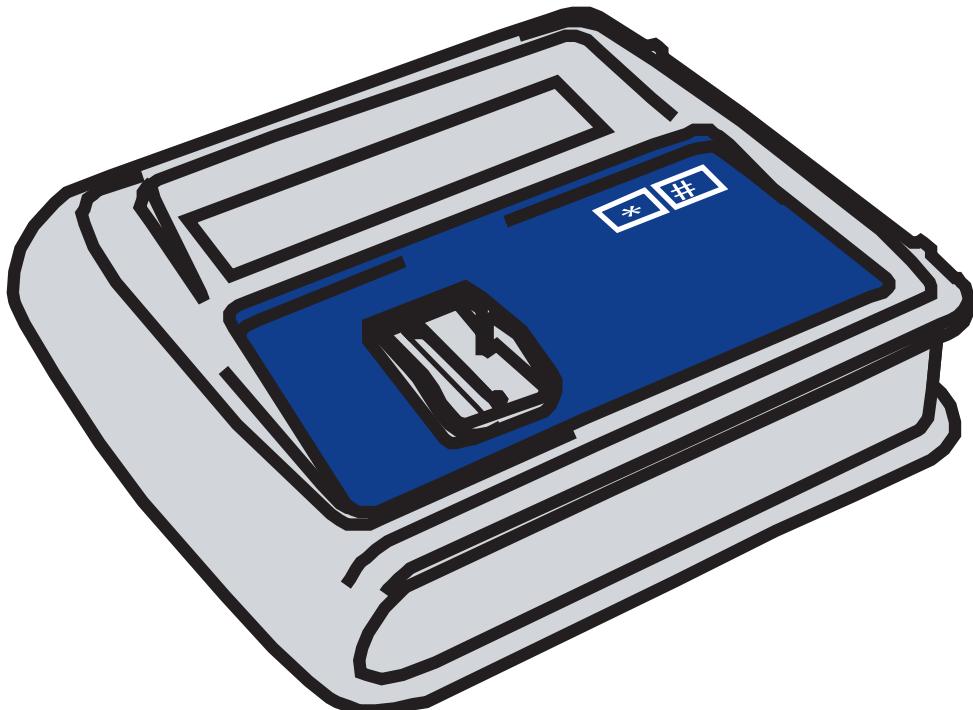

Use the Palintest DigiPAsS – fully portable  
field device giving accurate digital read-out  
between 2 and 100µg/l (ppb).